



## AC AUTOMATIC INSULATION/ WITHSTANDING HiTESTER 3174

Safety Standards  
Measuring Instruments



### Featuring contact check functionality

The effects of test lead wire breaks, erroneous test results caused by faulty contact, and fluctuations in test voltage caused by variations in the instrument's supply voltage on withstanding voltage and insulation resistance testing are well known.

The 3174 (3174-01) AC AUTOMATIC INSULATION/WITHSTANDING HiTESTER is a **low-cost solution featuring contact check functionality as well as a stabilized power supply** to prevent the reduced test reliability that can result from these issues.

To streamline production line test processes, the HiTESTER also features configuration of test parameters via RS-232C (GP-IB) and reading of parameters from the EXT I/O interface.



ISO 9001  
JMI-0216



ISO 14001  
JQA-E-90091



[www.hioki.com](http://www.hioki.com)

HIOKI company overview, new products, environmental considerations and other information are available on our website.


# Improved Test Reliability

**NEW**

## ● Contact check function improves test reliability


The 3174's contact check function lets you **detect test lead wire breaks and faulty contact** during testing by sensing measurement issues in real time.

◆ If a test lead wire were to break during testing with a tester that does not offer contact check functionality, defective test pieces would be judged to be non-defective.

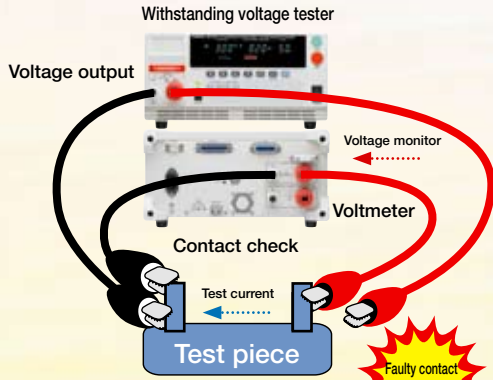

The 3174 improves test reliability by monitoring voltage to detect loose leads during testing and faulty wiring during measurement.

\*Since contact check is performed while testing is in progress, use of contact check functionality does not increase cycle time.

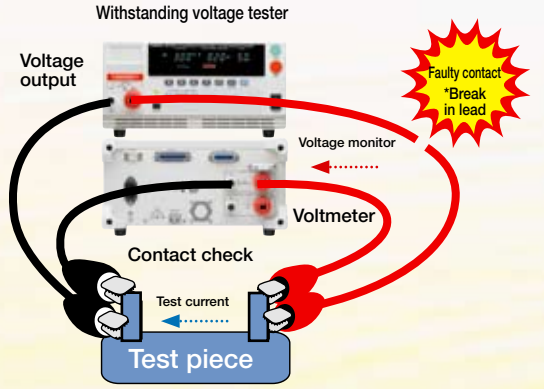

◆ If a test lead were to come loose during testing with a measurement device that does not offer contact check functionality, defective test pieces would be judged to be non-defective.

## DANGER lamp

Flashes a warning during testing and whenever high voltage is present at the terminals.  
The DANGER lamp turns off when the voltage at the output terminals is no greater than AC 30 V or DC 60 V.



9613  
SINGLE-HAND  
REMOTE CONTROL  
(option)

9614  
TWO-HAND  
REMOTE CONTROL  
(option)

## External switch

Enables start/stop control by means of the 9613 SINGLE-HAND REMOTE CONTROL or 9614 TWO-HAND REMOTE CONTROL.  
(The 9613 and 9614 are optional.)

## Test mode selection

Select from three test modes:  
1. Manual test mode: W (withstand voltage testing) / I (insulation resistance testing)  
2. Automatic test mode: W → I / I → W

Fluorescent display tube  
The display uses a bright, easy-to-read fluorescent tube.



**NEW**

## ● Judgment output at forced stop

The ability to obtain a judgment even after a forced stop increases testing freedom.

**NEW**

## ● Continued analytical testing after FAIL judgments

Test pieces can now be analyzed by means of detailed monitoring of the test current accompanying FAIL judgments.

## ● Ramp timer function

The ramp-up initial value, ramp-up and ramp-down time parameters can be set independently.

## ● True effective value display

## ● Eliminate the effects of supply voltage fluctuations

## ● Delay timer function



# Safe, Automated Operation

## Convenient


- Continuous full-auto withstanding voltage and insulation resistance testing

The 3174 lets you **set independent test conditions including test voltage for withstanding voltage and insulation resistance testing**, and you can perform these tests continuously. Press the W→I key to automatically perform withstanding voltage followed by insulation resistance tests, or press the I→W key to automatically perform insulation resistance followed by withstanding voltage tests.

## Safe

- Interlock function

Signal input from an external device such as an automatic tester can be used to disable output and prevent testing, **ensuring safety during automatic testing and other uses.**

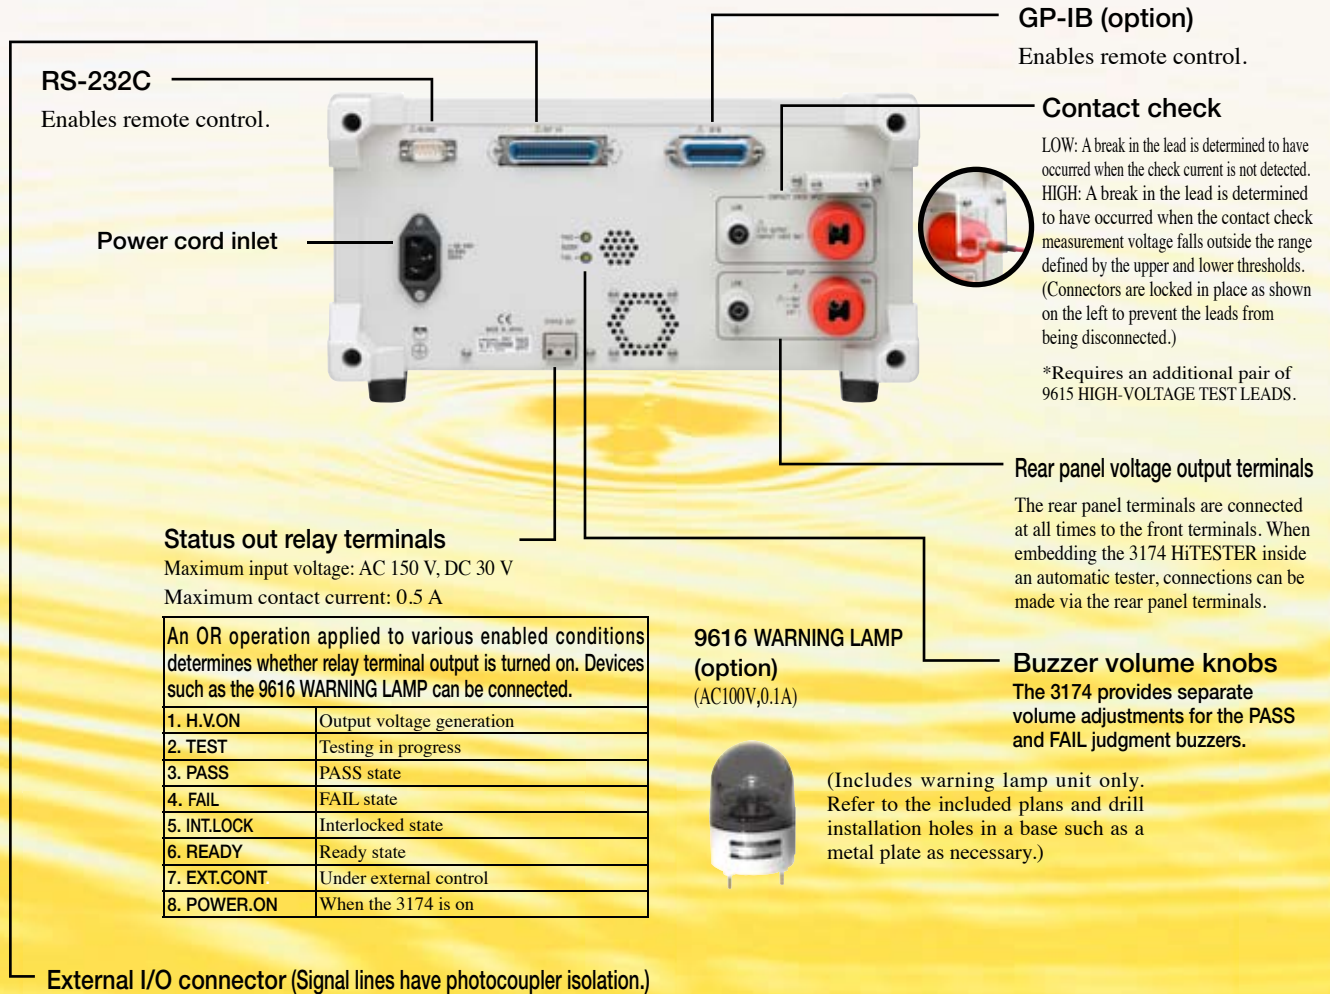

Pin	I/O	Signa	Function
1	OUT	READY	Low in ready state
2	OUT	L-FAIL	Low in FAIL state (lower bound)
3	OUT	U-FAIL	Low in FAIL state (upper bound)
4	OUT	PASS	Low in PASS state
5	OUT	TEST	Low in test state
6	OUT	H.V.ON	Low when voltage is present at output terminals
7	IN	EXT-E	When low, external I/O input signals are enabled
8	IN	START	When low, same function as START key
9	IN	STOP	When low, same function as STOP key
10	IN	INT.LOCK	Interlock on open
11	OUT	W-MODE	Low during withstanding voltage testing
12	OUT	I-MODE	Low during insulation resistance testing
13	OUT	W-FAIL	Low in FAIL state during withstand voltage testing
14	OUT	I-FAIL	Low in FAIL state during insulation resistance testing
15-18	IN	ISO.COM	Ground inputs for external devices
22-25	IN	MEM-0 to 3	Saved test selected pins
27	IN	MEM-E	When low, enables memory selected pins
28-29	OUT	MODE-0,1	Current test mode
33-36	OUT	ISO.DCV	Internal DC 15 V power supply (100 mA)

## Interface specifications

### EXT I/O : Output signals

Open collector output (with photocoupler isolation)  
All active low with a maximum load voltage of DC 30 V  
Maximum output current: DC 100 mA per signal  
Output saturation voltage: DC 1.5 V or less

### Input signals

All active low input (with photocoupler isolation)  
Maximum applied voltage: 30 V  
High level voltage: from DC 15 V to 30 V, or open  
Low level voltage: DC 5 V or less (-6 mA typ.)

### EXT SW : Input signals (contact input)

START, STOP, SW.EN (external switch terminal enable)

### Output signals

LED activation signal (maximum load current: 40 mA)

## Withstanding Voltage Testing

### [ Test Voltage ]

<b>Output voltage</b>	: AC 0.2 to 5 kV (50/60 Hz), single-range output
<b>Voltage output method</b>	: PWM switching method (0 V start; voltage can be changed while generating output)
<b>Voltage specification method</b>	: Digital (setting resolution: 0.01 kV)
<b>Output voltage accuracy</b>	: $\pm 1.5\%$ of setting $\pm 20$ V
<b>Maximum rated output</b>	: AC 100 VA (5 kV/20 mA) continuous rating
<b>Transformer capacity</b>	: 100VA
<b>Voltmeter</b>	: True effective value display Digital meter: AC 0 kV to 5.00 kV Accuracy: $\pm 1.5\%$ rdg (1,000 V or less, $\pm 15$ V)
<b>Output waveform</b>	: Sine wave
<b>Voltage change rate</b>	: 15% or less (converges to setting within 1 s during change from maximum rated load to no load)
<b>Distortion factor</b>	: 5% or less (tester impedance during measurement with 5 kV output under 40 M $\Omega$ load)
<b>Frequency</b>	: 50/60Hz ( $\pm 0.2\%$ )

### [ Current Detection ]

<b>Current measurement range</b>	: 0.01 mA to 20 mA (2 ranges)
<b>Measurement range</b>	: 10mA/20mA
<b>Indicated value</b>	: True effective value display
<b>Measurement ranges and resolutions</b>	: 0.00 mA to 10.00 mA, 0.01 mA (10 mA range) 0.0 mA to 20.0 mA, 0.1 mA (20 mA range)
<b>Measurement accuracy</b>	: $\pm 2\%$ rdg $\pm 0.05$ mA (10 mA range) $\pm 2\%$ rdg $\pm 0.5$ mA (20 mA range)

## Insulation Resistance Measurement

### [ Test Voltage ]

<b>Rated voltage</b>	: DC 500 V/1,000 V (positive polarity)
<b>Unloaded voltage</b>	: 1 to 1.2 times rated voltage
<b>Rated measurement current</b>	: 1 to 1.2 mA
<b>Short-circuit current</b>	: 4 to 5 mA (500 V), 2 to 3 mA (1,000 V)
<b>Measurement range</b>	: 0.2 to 2,000 M $\Omega$ (500 V), 0.5 to 2,000 M $\Omega$ (1,000 V)
<b>Guaranteed accuracy ranges/accuracies</b>	: 0.5 to 999 M $\Omega$ (500 V), 1 M $\Omega$ to 999 M $\Omega$ (1,000 V): $\pm 4\%$ rdg 1,000 M $\Omega$ to 2,000 M $\Omega$ : $\pm 8\%$ rdg
<b>Measurement resolution</b>	: 0.01 M $\Omega$ (0.20 M $\Omega$ to 19.9 M $\Omega$ ) 0.1 M $\Omega$ (20.0 M $\Omega$ to 199.9 M $\Omega$ ), 1 M $\Omega$ (200 M $\Omega$ to 2,000 M $\Omega$ )
<b>Measured resistance ranges</b>	: 2 M $\Omega$ , 20 M $\Omega$ , 200 M $\Omega$ , 2,000 M $\Omega$ (500 V) 4 M $\Omega$ , 40 M $\Omega$ , 400 M $\Omega$ , 2,000 M $\Omega$ (1,000 V)

## General Specifications

<b>Display</b>	: Fluorescent display tube (digital display)
<b>Monitor functions</b>	: Output voltage, detected current, insulation resistance
<b>Monitor period</b>	: 2 times per second, minimum
<b>Operating temperature range</b>	: 0°C to 40°C, 80% RH or less (non-condensing)
<b>Storage temperature range</b>	: -10°C to 50°C, 90% RH or less (non-condensing)
<b>Temperature and humidity range for guaranteed accuracy</b>	: 23 $\pm$ 5°C, 80% RH or less (non-condensing) (With warm-up period of at least 10 min)
<b>Guaranteed accuracy term</b>	: 1 year
<b>Operating environment</b>	: Indoors at elevations of up to 2,000 m at a pollution level of 2
<b>Supply voltage</b>	: AC 100 to 240 V Designed to tolerate voltage fluctuations of $\pm 10\%$ of the rated supply voltage.
<b>Power supply frequency</b>	: 50Hz/60Hz
<b>Withstanding voltage</b>	: Power supply to chassis: 1.39 kV at 10 mA for 15 s
<b>Maximum rated power</b>	: 200VA
<b>Dimensions</b>	: Approx. 320 (W) $\times$ 155 (H) $\times$ 395 (D) mm (excluding protruding parts)
<b>Weight</b>	: Approx. 15 kg
<b>Applicable standards</b>	: EMC: EN61326 Class A, EN61000-3-2, EN61000-3-3, Safety: EN61010-1
<b>Included accessories</b>	: HIGH-VOLTAGE TEST LEADS 9615 (1 each high-voltage and return), power cord, disconnection prevention plate

# HIOKI

HIOKI E. E. CORPORATION

#### HEAD OFFICE :

81 Koizumi, Ueda, Nagano, 386-1192, Japan  
TEL +81-268-28-0562 / FAX +81-268-28-0568  
E-mail: os-com@hioki.co.jp

#### HIOKI USA CORPORATION :

6 Corporate Drive, Cranbury, NJ 08512 USA  
TEL +1-609-409-9109 / FAX +1-609-409-9108  
E-mail: hioki@hiokiusa.com

#### HIOKI (Shanghai) Sales & Trading Co., Ltd. :

1904 Shanghai Times Square Office, 93 Huai Hai Zhong Road  
Shanghai, P.R.China POSTCODE: 200021  
TEL +86-21-6391-0090/0092 FAX +86-21-6391-0360  
E-mail: info-sh@hioki.cn

#### Beijing Office :

A-2602 Freetown, 58 Dong San Huan Nan Road  
Beijing, P.R.China POSTCODE: 100022  
TEL +86-10-5867-4080/4081 FAX +86-10-5867-4090  
E-mail: info-bj@hioki.cn

#### Guangzhou Office :

Room 303, Profit Plaza, No.76, West Huangpu Road  
Guangzhou, P.R.China POSTCODE: 510623  
TEL +86-20-38392673/2676 FAX +86-20-38392679  
E-mail: info-gz@hioki.cn

## Timers

<b>Setting range</b>	: 0.3 to 999 s
<b>Operation</b>	: When set to on: Display counts down from the set time after start. When set to off: Display indicates time elapsed since start.
<b>Setting resolution/accuracy</b>	: 0.1 s (0.3 to 99.9 s) $\pm 50$ ms 1 s (100 to 999 s) $\pm 0.5$ s

### [ Ramp Timers ] (Withstand voltage testing)

<b>Setting range</b>	: 0.1 to 99.9 s: Ramp-up and ramp-down can be set independently.
<b>Operation</b>	: Ramp-up: The output voltage increases linearly from the initial voltage to the test voltage over the ramp-up time. Ramp-down: The output voltage decreases from the set voltage to 0 V over the ramp-down time after the test time elapses, and the display counts down from the set time. *The actual ramp-up waveform varies with the load due to the analog response delay.
<b>Setting resolution</b>	: 0.1s

### [ Delay Timers ] (Insulation resistance testing)

<b>Setting range</b>	: 0.1 to 99.9 s
<b>Setting resolution</b>	: 0.1s

## Decision Function

<b>Decision method</b>	: Window comparison method with upper and lower bound settings (digital specification)
<b>Decision results</b>	: UPPER-FAIL: The measured current (measured insulation value) exceeded the specified upper threshold. PASS: The measured current (measured insulation value) fell within the range defined by the specified upper and lower thresholds. LOWER-FAIL: The measured current (measured insulation value) was less than the specified lower bound. UPPER LOWER-FAIL: A testing error occurred, for example due to a failure to generate the set voltage.
<b>Decision processing</b>	: Display, buzzer, and EXT I/O signal output is generated according to each decision result.
<b>Setting range</b>	: AC withstanding voltage: 0.1 to 20.0 mA (upper threshold), 0.1 to 19.9 mA (lower threshold) DC insulation: 0.2 to 2,000 M $\Omega$ (500 V) or 1.0 to 2,000 M $\Omega$ (1,000 V) for both upper and lower thresholds
<b>Setting resolution</b>	: AC withstanding voltage: 0.1 mA DC insulation: 0.01 M $\Omega$ (0.2 to 2.00 M $\Omega$ ), 0.1 M $\Omega$ (2.10 to 20.0 M $\Omega$ ), 1 M $\Omega$ (21.0 to 200 M $\Omega$ ), 10 M $\Omega$ (210 to 2,000 M $\Omega$ )

## Contact Check

<b>Voltmeter accuracy</b>	: Detection method: Average value detection/effective value conversion Accuracy: Setting $\pm 50$ V *Inaccuracy may increase when the waveform is distorted.
<b>Decision results</b>	: Enables the contact check function (does not increase cycle time). LOW: A break in the lead is determined to have occurred when the check current is not detected. HIGH: Upper and lower thresholds for the check detection voltage can be set. A break in the lead is determined to have occurred when the contact check measurement voltage falls outside the range defined by the upper and lower thresholds.
<b>Voltage setting range</b>	: Withstanding voltage testing: 0.20 kV to 5.0 kV (0.01 kV resolution; applies to both upper and lower thresholds) Insulation resistance measurement: Upper threshold of 600 V and lower threshold of 500 V (during 500 V measurement); upper threshold of 1,200 V and lower threshold of 1,000 V (during 1,000 V measurement) (both fixed)

## Model

AC AUTOMATIC INSULATION/WITHSTANDING HITESTER 3174
AC AUTOMATIC INSULATION/WITHSTANDING HITESTER 3174-01 (GP-IB Model)

## Options

ELECTRIC SAFETY TESTING SOFTWARE	9267 (available soon)
SINGLE-HAND REMOTE CONTROL	9613
TWO-HAND REMOTE CONTROL	9614
HIGH-VOLTAGE TEST LEADS	9615
WARNING LAMP (AC100V,0.1A)	9616
RS-232C CABLE (9-pin to 9-pin/cross/1.8 m)	9637
RS-232C CABLE (9-pin to 25-pin/cross/1.8 m)	9638
GP-IB CONNECTING CABLE (2 m)	9151-02